

Figure 1

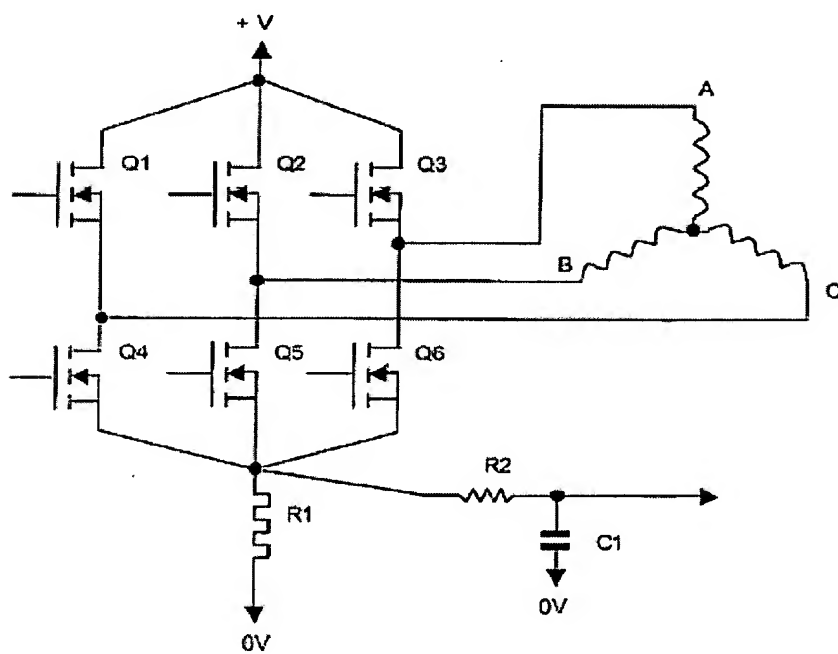


Figure 2

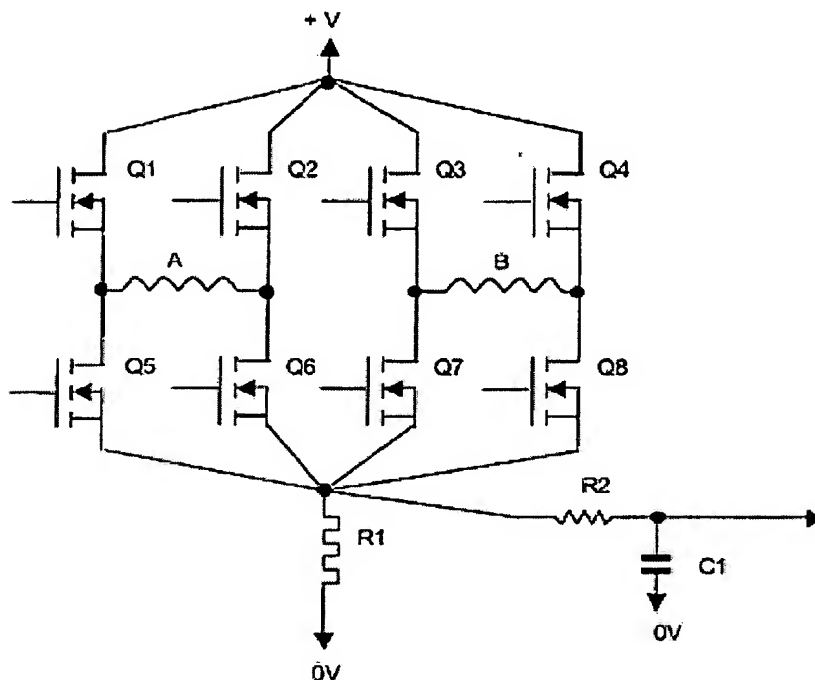


Figure 3

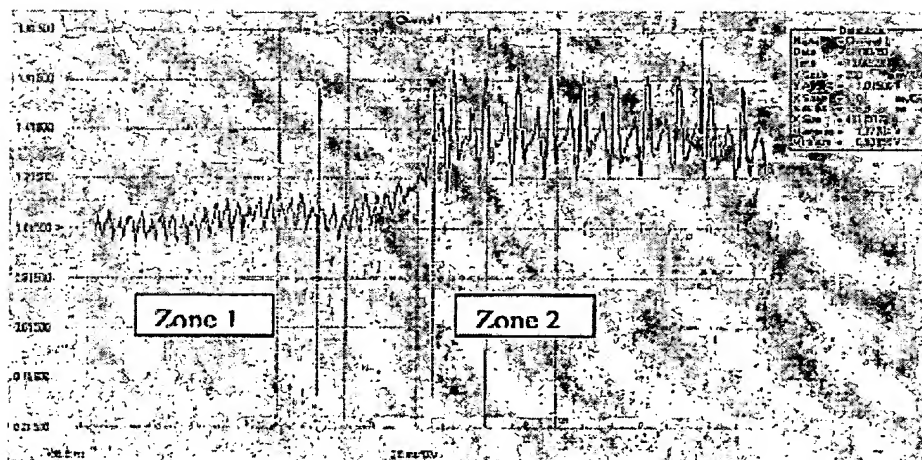


Figure 4


BEST AVAILABLE COPY

Fig. 5: [poorly legible]

Analysis of the standard deviation for a depth of 32 samples – sampling period = 0.0002 s

Real current with end stop
Deviation No.

Current (U 1023)

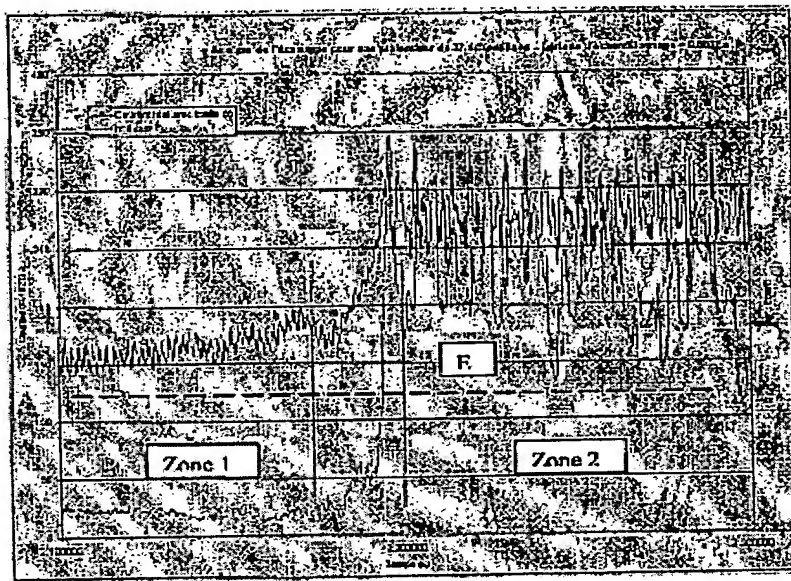

Deviation No.

Time (s)

Figure 5

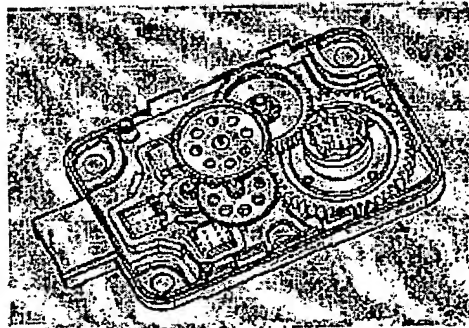


Figure 6

BEST AVAILABLE COPY

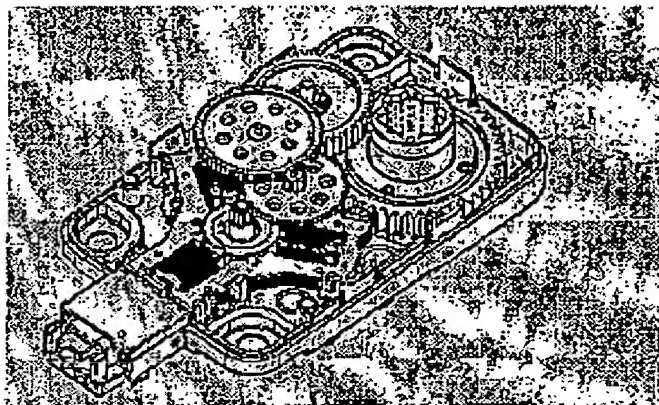


Figure 7

BEST AVAILABLE COPY